

TEST REPORT



No:200048255

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: USRC-2089-24



ISSUE DATE:2020-03-28

APPLICANT: Shenzhen loee Biotechnology Co.,Ltd
ADDRESS: A-111,xixiangBaoan, shenzhen

APPLICANT PROVIDED SAMPLE DESCRIPTION:

Twenty(20) Pieces of Seif-imbibition Filter Respirator Against Particulate Matter

BRAND: LOEE

COLOUR: White

SIZE: LOEE9510

MANUFACTURE' S NAME: Lueyang loee Medical Technlogy Co.,Ltd

DATE RECEIVED/DATE TEST STARTED: 2020-03-24

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER M

INSPIRATORY RESISTANCE M

EXPIRATORY RESISTANCE M

NOTE: "M" -MEET THE STANDARD' S REQUIREMENT "F" -FAIL TO MEET THE STANDARD' S REQUIREMENT
"—" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200048218.

ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).

COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.

THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:
Nan Ma ENGINEER


马楠



PAGE 1 OF 3

TEST REPORT

No: 200048255

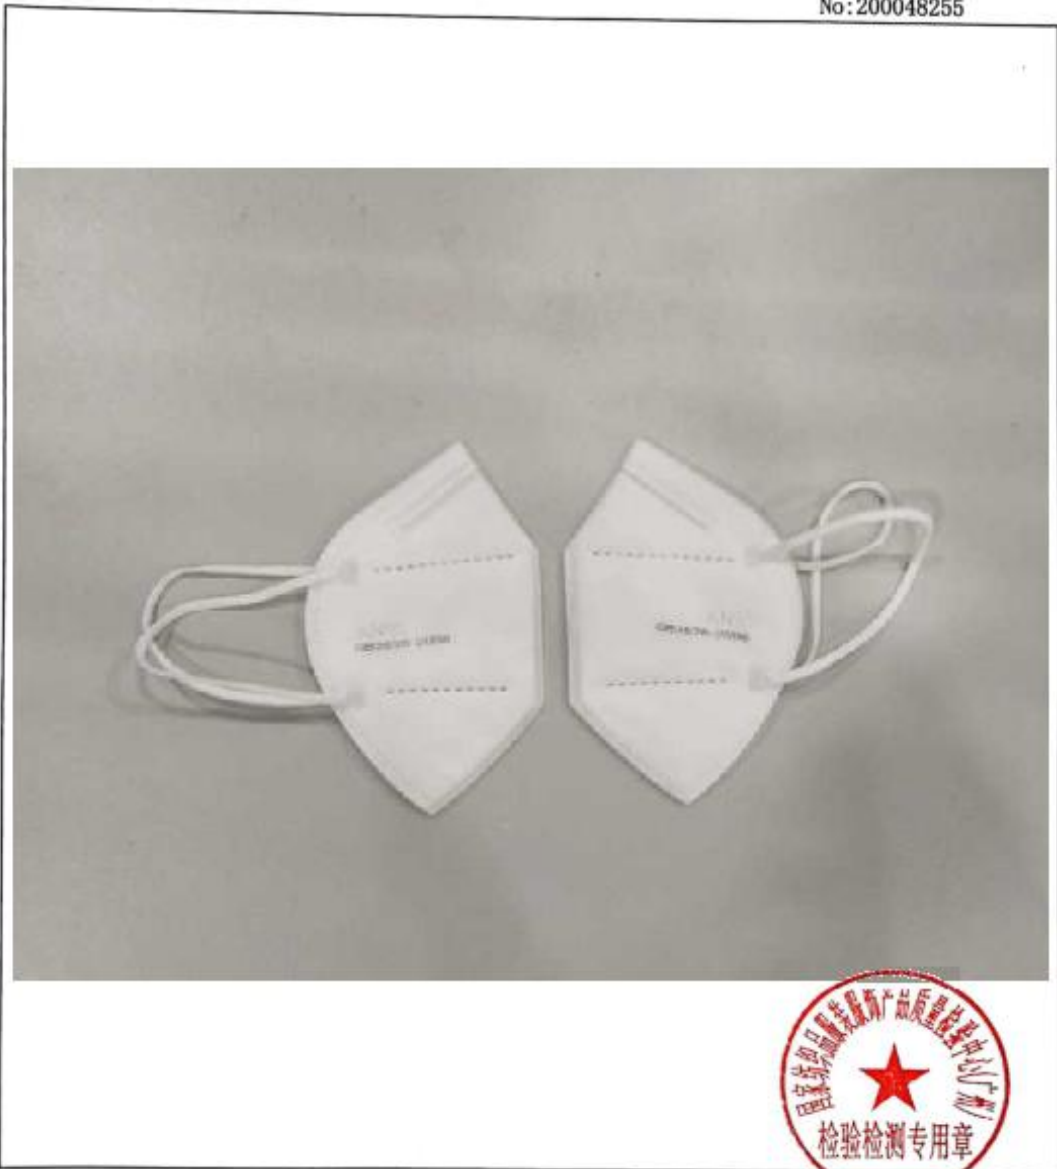

PAGE 2 OF 3

TEST REPORT

No: 200048255

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW: 85L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION: 15mg/m³, TEMP: 24.1°C, RH: 38.3%)

FILTRATION EFFICIENCY (%):

UNTREATED SAMPLE

1# 96.73
2# 95.89
3# 96.71
4# 96.52
5# 95.87
6# 96.41
7# 96.87
8# 96.01
9# 96.27
10# 96.44

CONDITIONING TREATED

1# 95.21
2# 95.81
3# 95.60
4# 95.19
5# 95.73

REQUIREMENT

FILTRATION EFFICIENCY (%):

≥ 95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 118.2
2# 114.7

PRETREATMENT SAMPLE:

1# 98.5
2# 103.2

REQUIREMENT

≤ 350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 87.6
2# 93.1

PRETREATMENT SAMPLE:

1# 90.2
2# 83.7

REQUIREMENT

≤ 250
(GB 2626-2006)



—End of Report—

PAGE 3 OF 3